

Title:

Effect of Contact Lens Surface Properties on Comfort, Tear Stability and Ocular Physiology

Author names:

Maria Vidal-Rohr^{1,2}; James S. Wolffsohn^{1*}, Leon N. Davies¹, Alejandro Cerviño²

Author affiliations:

1. Ophthalmic Research Group, Aston University, Aston Triangle, Birmingham, B4 7ET, UK

2. Optometry Research Group, University of Valencia, Burjassot, 46100, ES

*** Corresponding author:**

At: Ophthalmic Research Group, Aston University, Aston Triangle, Birmingham, B4 7ET, UK

E-mail address: j.s.w.wolffsohn@aston.ac.uk

Tel.: +44 0121 204 4140

Abstract

Aim: Retrospective analysis of different contact lens wearing groups suggests lens surface lubricity is the main factor influencing contact lens comfort. However, the commercially available contact lenses examined differ in material and design as well as surface properties. Hence this study isolates the contribution of lens surface properties using an ultra-thin coating technology.

Methods: Nineteen habitual contact lens wearers (21.6 ± 1.7 years) wore formofilcon B soft monthly disposable contact lenses with and without coating technology modified surface properties for a month each in a randomised double-masked cross-over study. Objective non-invasive breakup time (NIKBUT), NIKBUT average and ocular redness (Jenvis grading scale) were evaluated (Keratograph 5M) after 1 week and 1 month of wear. Symptoms were assessed using the Contact Lens Dry Eye Questionnaire (CLDEQ-8); perceived vision quality and subjective lens comfort at insertion, mid-day and end of the day were rated with Visual Analog Scales.

Results: Perceived visual quality ($F=5.049, p=0.037$), contact lens dry eye symptoms ($F=14.408, p=0.001$) and subjective lens comfort ($F=28.447, p<0.001$) were better for coated compared to uncoated lenses. The surface coating postponed the lens dewetting ($F=8.518, p=0.009$) and increased the pre-lens tear film stability ($F=5.626, p=0.029$), but bulbar ($F=0.340, p=0.567$) and limbal ($F=0.110, p=0.744$) redness were similar for both contact lenses. No parameter changed significantly between a weeks' and months' wear ($p>0.05$). Lens surface wettability and ocular redness were not correlated to changes in symptoms ($p>0.05$).

Conclusion: As previously hypothesised, changing the physical surface properties of a soft contact lens improves subjectively rated wearer comfort, which, in turn, should result in reduced contact lens discontinuation.

Keywords:

Discomfort; coating; soft contact lens; tear film; lubricity; coefficient of friction

Highlights:

- Retrospective analysis suggests contact lens surface lubricity influences comfort.
- Previous results are confounded by differences in material and design.
- This study isolates the contribution of lens surface properties using a coating.
- The surface coating improved wettability and increased lubricity. Coated lenses were more comfortable, without affecting ocular physiology.
- This study suggests the importance of considering the coefficient of friction when fitting a contact lens.

Introduction

The management of contact lens discomfort (CLD) remains a challenge in clinical practice (1). There are more than 140 million contact lens wearers worldwide and about 50% of them report having adverse ocular sensations (1, 2), generally described as ocular dryness (3, 4).

The insertion of a contact lens into the eye includes various factors that may be related to CLD. Ocular dryness decreases after lens removal, (5) and generally reduces during the afternoon and evening when wearing contact lenses (4-8). Moreover, dry eye symptoms in contact lens wearers are more frequent and intensive than those of non-contact lens wearers (9-10). Replacing the lens midway through the wearing period does not improve end of day comfort, suggesting that the physical presence of the lens and its interaction with the ocular surface causes a fatiguing effect on ocular tissues or stimulates nociceptors, rather than the decrease in comfort is due to changes occurring to the lenses during wear (11). To diagnose CLD, the integrity of the tear film (12-15) and meibomian glands (16) as well as the ocular redness (17) and staining (18-20) are typically assessed. Nevertheless, the correlation between these signs and dry eye symptoms is generally poor (21).

Research in CLD aims to determine which contact lens properties (e.g. design and material) will improve contact lens adaptation. Hydrogels with lower water content have been shown to have greater lens hydration (22, 23), providing a better lens comfort (24, 25) than higher water content materials. Attempts to extend lens wear by increasing lens oxygen permeability have been addressed by adding silicone components to hydrogel materials (26). However, silicone-containing monomers compromise lens wettability, giving rise to strategies to make silicone hydrogels more hydrophilic (26). Current studies have suggested that the friction between lens surface and lid margin (termed lubricity) is the key contributor to lens comfort (26-29); however, they use commercially available contact lenses which differ in material and design and are generally worn by different cohorts of patients, introducing potential confounding effects.

This study applied a nanometer thickness coating technology (without significantly altering lens design or core material properties) to monthly disposable silicone hydrogel lenses to determine whether surface properties alone affect lens comfort and wettability.

Method

Twenty habitual contact lens wearers were recruited for a randomised double-masked cross-over wear of formofilcon B monthly disposable soft contact lenses of the same design and modulus, with and without modifying the surface properties with a coating technology (Bettersvision Pty, Keller, TX, USA; Table 1). A modified CSM nano-scratch tribometer was used to measure the dynamic coefficient of friction (CoF). Consent was obtained after explanation of the study and possible consequences of taking part. The study was approved by the ethical committee of Aston University, and conformed to the tenets of the Declaration of Helsinki. Participants were excluded from the study if they had astigmatism $\geq 0.75D$, a best corrected visual acuity of >0.1 logMAR, had any ocular or systemic disease or surgery which might interfere with contact lens wear, were on medication with known ocular side effects, or were pregnant or breast feeding. Inclusion criteria included being ≥ 18 years of age and having a healthy ocular surface (Jenvis grades ≤ 2). All subjects expressed a desire to wear contact lenses full time and agreed to wear their lenses for a minimum of 7 hours per day throughout the study. The subjects were masked to the prescribed contact lenses. They were provided with a supply of hydrogen peroxide solution and case (AOSept Plus, Alcon, Fort Worth, USA) and were talked through the cleaning regimen including neutralising, rubbing and rinsing. No additional solutions or eye drops could be used throughout the study. Moreover, contact lens fit was adequate and evaluated in each visit using a simplified recording scheme (30).

A clinical evaluation was conducted one week and one month after wearing each contact lens type, bilaterally in randomised order, each for one month. Objective non-invasive break up time (NIKBUT), the average time of all break up incidents (NIKBUT average), and nasal and temporal bulbar and limbal redness (Jenvis grading scale) were evaluated in both eyes after at least one hour of lens settling and with the Keratograph 5M (OCULUS Optikgeraete GmbH, Wetzlar, Germany), previously shown to be repeatable (31). Three consecutive NIKBUT and NIKBUT average readings were taken separated by at least 60 seconds and the mean was recorded. Contact lens dry eye symptoms were assessed using the 8-item Contact Lens Dry Eye Questionnaire (CLDEQ-8). Moreover, perceived vision quality and subjective lens comfort between visits were separately rated at insertion, mid-day and end of the day using four different Visual Analog Scales (VAS).

Statistical analysis

The data were continuous and normally distributed (confirmed using the Kolmogorov-Smirnov test) hence parametric statistics were utilised. Repeated measure analysis of variance (ANOVA) testing (with coating, duration of wear, eye and nasal and temporal quadrants as factors) was performed to establish whether a statistically significant difference ($p < 0.05$) existed between NIKBUT, NIKBUT

average, comfort and ocular redness measured for coated and uncoated contact lenses. Mauchly's Test of Sphericity was used to test the assumption of sphericity; in case of sphericity violation, Greenhouse-Geisser correction was applied. The association between subjective symptoms of ocular dryness and lens surface tear stability was assessed with a Pearson's correlation. Due to the repeated measures design, at least 15 degrees of freedom is recommended (32), which was achieved with a sample size ≥ 15 .

Table 1: Contact lens characteristics with and without the coating technology (mean \pm S.D.).

PARAMETER	MEASUREMENT	
	Uncoated Lenses	Coated Lenses
Modulus (MPa)	0.42 \pm 0.19	0.45 \pm 0.15
Sessile-drop Contact Angle (°)	42 \pm 15	61 \pm 11
Coefficient of friction	0.071 \pm 0.005	0.004 \pm 0.003
Water Content (%)	50	
Dk/t (@ -3.00D) (barrer/mm)	140	
Diameter (mm)	14.2	
Base curve (mm)	8.6	
Center Thickness (μ m)	80	
UV filtration	Class 1 Blocking	
Coating (nm)	< 6 - 10	

Results

Nineteen subjects (21.6 ± 1.7 years, 17 females) successfully finished the study. The drop out was due to the individual's scheduling issues. No adverse events occurred during the study. Perceived visual quality ($F=5.049$, $p=0.037$; Figure 1), contact lens dry eye symptoms ($F=14.408$, $p=0.001$; Figure 2) and subjective lens comfort ($F=28.447$, $p < 0.001$; Figure 3) were better for coated lenses compared to uncoated lenses, with no significant changes between a weeks' and months' wear ($F=4.122$, $p=0.057$; $F=0.558$, $p=0.465$; $F=3.137$, $p=0.72$, respectively). Tear film stability of the contact lens anterior surface and NIKBUT average were longer with coated lenses ($F=5.626$, $p=0.029$; $F=8.518$, $p=0.009$, respectively), was bilaterally similar ($F=0.571$, $p=0.460$; $F=0.058$, $p=0.820$, respectively) and was stable between one week and one month of lens wear ($F=2.748$, $p=0.115$; $F=0.673$, $p=0.423$, respectively; Table 2). Bulbar redness did not significantly differ with contact lens coating ($F=0.340$, $p=0.567$), between one week and one month of wear ($F=0.057$, $p=0.814$), right and left eyes ($F=3.992$, $p=0.615$) or nasal and temporal quadrants ($F=0.049$, $p=0.818$). This was also the case with limbal redness, with no significant differences with the contact lens coating ($F=0.110$, $p=0.744$), between one week and one month of wear ($F=0.261$, $p=0.615$) or between eyes ($F=0.123$, $p=0.730$), although the nasal limbus was significantly redder than the temporal limbus (0.25 ± 0.23 vs 0.18 ± 0.20 ; $F=6.449$, $p=0.021$). In addition, there was no interaction between factors when analysing differences between NIKBUT, NIKBUT average, comfort and ocular redness measured for coated and uncoated contact lenses ($p>0.05$). Subjectively rated ocular dryness in coated and non-coated contact lenses was not correlated with lens surface wettability, NIKBUT average values or ocular redness (COATED: NIKBUT: $r=-0.198$, $p=0.417$; NIKBUT average: $r=-0.360$, $p=0.130$; Bulbar redness: $r=-0.137$, $p=0.575$; Limbal redness: $r=0.123$, $p=0.615$; UNCOATED: NIKBUT: $r=-0.321$, $p=0.180$; NIKBUT average: $r=-0.305$, $p=0.205$; Bulbar redness: $r=-0.124$, $p=0.612$; Limbal redness: $r=0.046$, $p=0.851$) or the change in an individual (NIKBUT: $r=0.140$, $p=0.568$; NIKBUT average: $r=-0.187$, $p=0.442$; Bulbar redness: $r=0.027$, $p=0.914$; Limbal redness: $r=-0.21$, $p=0.932$).

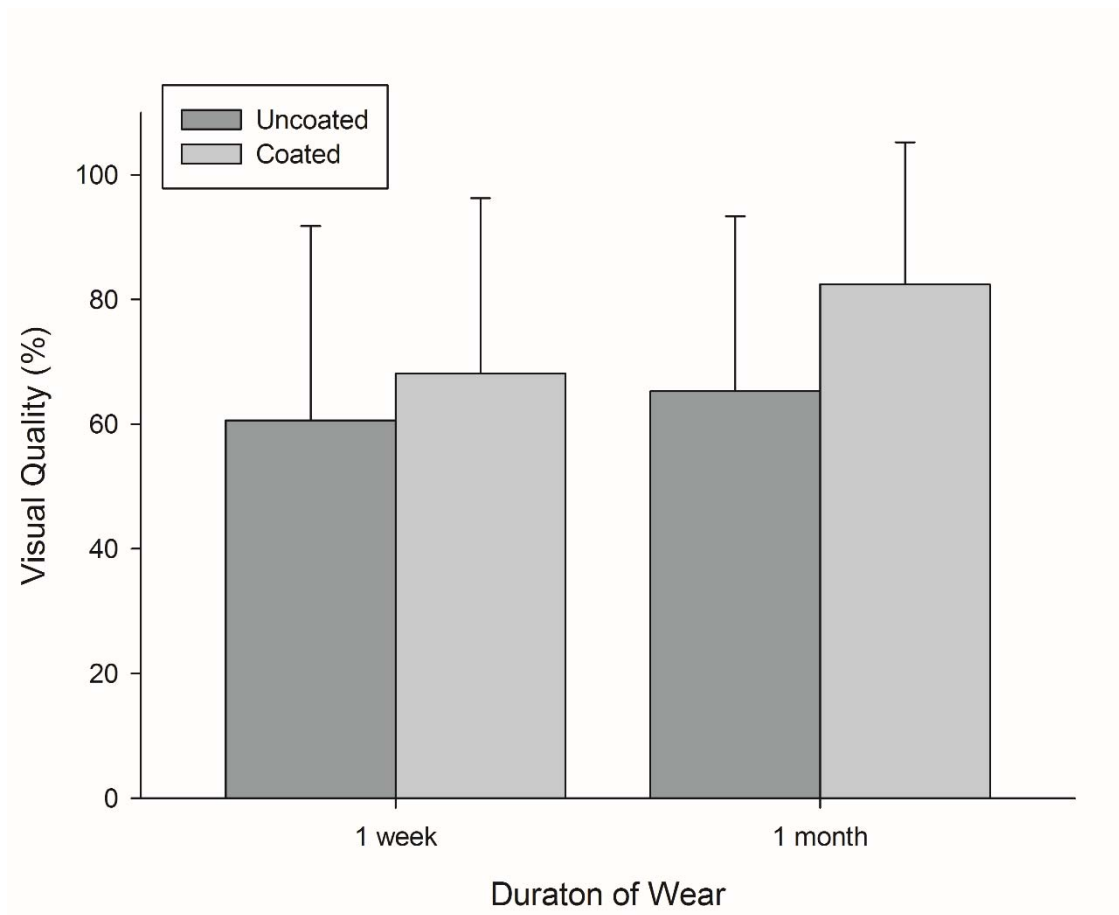


Figure 1: Subjectively rated visual quality with and without contact lens coating with duration of wear. N=19. Error bars = ± 1 S.D.

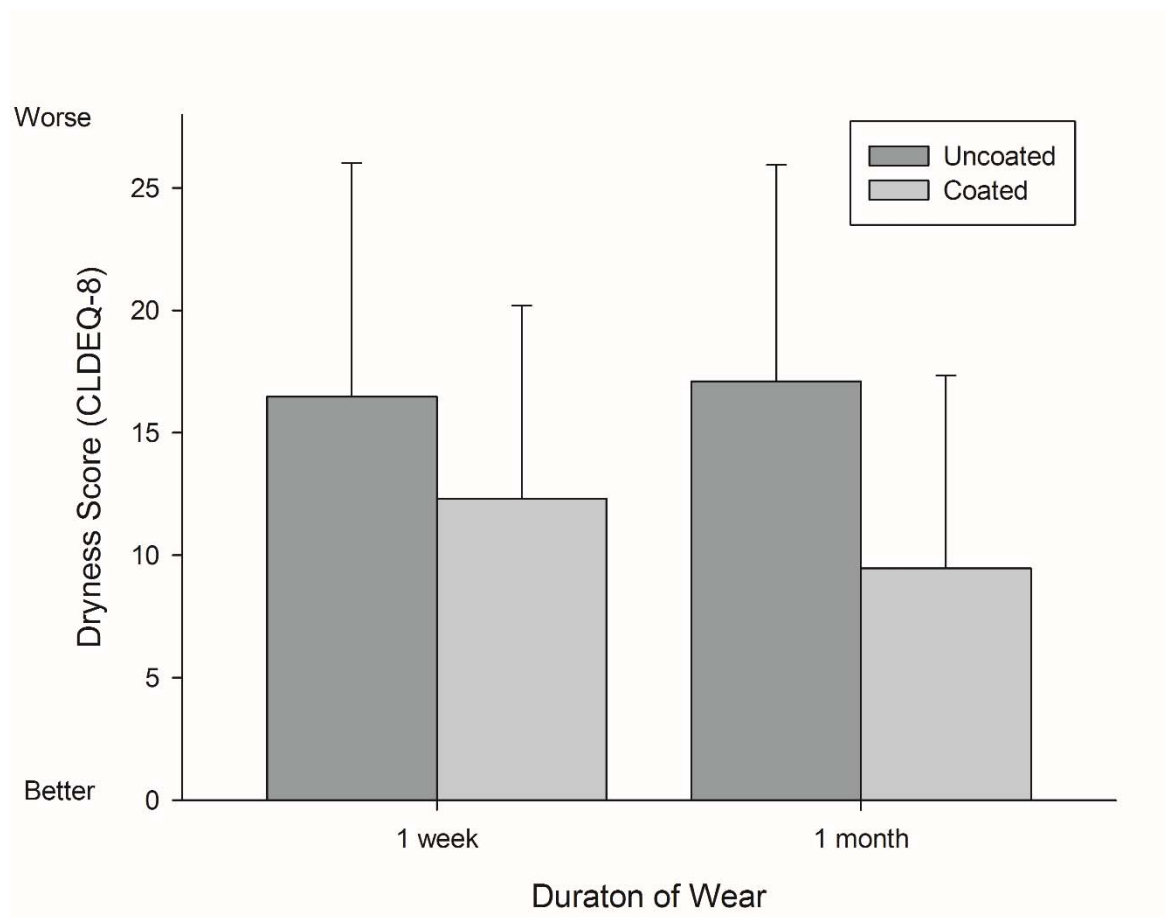


Figure 2: Dryness symptoms with and without contact lens coating with duration of wear. N=19. Error bars = ± 1 S.D.

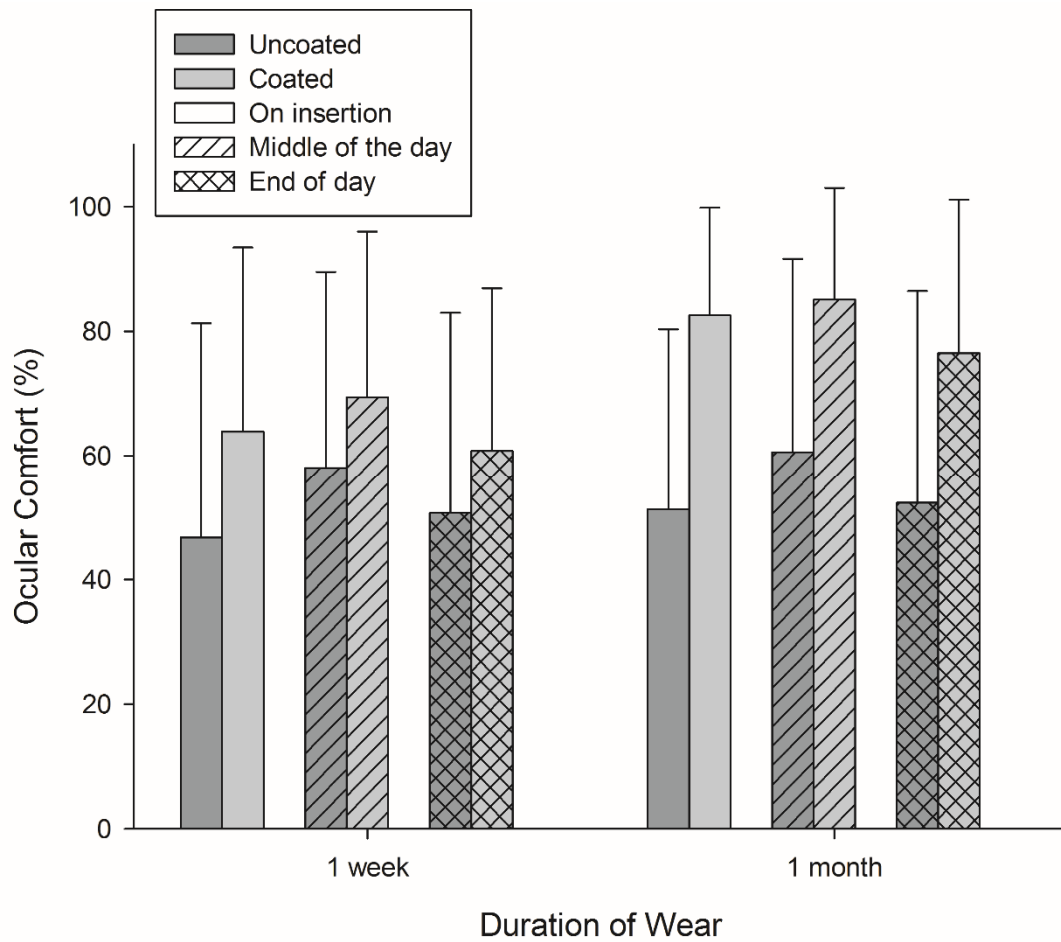


Figure 3: Ocular comfort with and without contact lens coating with time of day and duration of wear. N=19. Error bars = ± 1 S.D.

Variable		1 week wear		1 month wear	
		Uncoated Lenses	Coated Lenses	Uncoated Lenses	Coated Lenses
COMFORT (%)					
• Insertion		46.74 ± 34.53	63.89 ± 29.54	51.26 ± 29.04	82.53 ± 17.29
• Mid-day		58.05 ± 31.48	69.37 ± 26.60	60.58 ± 31.03	85.05 ± 17.94
• End-of-day		50.68 ± 32.29	60.79 ± 26.08	52.32 ± 34.15	76.47 ± 24.63
VISUAL QUALITY (%)					
Visual quality		60.63 ± 31.16	68.11 ± 28.15	65.26 ± 28.08	82.42 ± 22.81
DISCOMFORT (score)					
CLDEQ-8		16.47 ± 9.55	12.32 ± 7.88	17.11 ± 8.84	9.47 ± 7.87
NIK BUT (seconds)					
RE		5.05 ± 2.18	6.73 ± 3.26	5.86 ± 3.28	7.10 ± 3.95
LE		6.15 ± 3.86	6.13 ± 3.23	6.19 ± 3.44	8.45 ± 4.84
NIK BUT average (seconds)					
RE		11.39 ± 4.83	12.49 ± 4.79	12.86 ± 5.22	13.89 ± 4.92
LE		11.41 ± 6.31	13.68 ± 4.85	10.90 ± 5.58	14.05 ± 5.66
BULBAR REDNESS (grade)					
RE	N	0.51 ± 0.35	0.44 ± 0.19	0.47 ± 0.23	0.49 ± 0.33
	T	0.51 ± 0.25	0.44 ± 0.19	0.46 ± 0.19	0.56 ± 0.42
LE	N	0.56 ± 0.34	0.49 ± 0.21	0.57 ± 0.29	0.54 ± 0.21
	T	0.58 ± 0.25	0.52 ± 0.17	0.53 ± 0.15	0.51 ± 0.26
LIMBAL REDNESS (grade)					
RE	N	0.27 ± 0.30	0.21 ± 0.21	0.22 ± 0.18	0.29 ± 0.26
	T	0.23 ± 0.26	0.16 ± 0.14	0.16 ± 0.13	0.195 ± 0.24
LE	N	0.24 ± 0.27	0.22 ± 0.16	0.27 ± 0.23	0.31 ± 0.24
	T	0.25 ± 0.26	0.14 ± 0.12	0.16 ± 0.12	0.21 ± 0.25

Table 2: Comfort, tear film stability (NIK BUT=non-invasive keratoscope tear break-up time), NIK BUT average and ocular redness after 1 week and 1 month of wear of a silicone hydrogel contact lens with or without a surface coating. RE= right eye; LE= left eye; mean ± 1 S.D.; n=19.

Discussion

Commercial lens surface wettability has been increased through the application of coatings and surface moisturising agents with the purpose of increasing lens comfort (26). Brennan compared the coefficient of friction values from Ross et al. (27) with end-of-day comfort values from over 700 one-month wearing trials and demonstrated a significant correlation ($r^2 = 0.79$ $p < 0.01$) (28). The same analysis was conducted with a different source of coefficient of friction data (29) and showed a significant association between the coefficient of friction and end-of-day comfort ($r^2 > 0.83$, $p < 0.01$) (33). Nevertheless, the investigated lenses were commercially available and differed in design and material composition, confounding attempts to determine which physical properties are principally responsible for lens comfort (26).

The current investigation is the first to examine the isolated effect of reducing lens surface friction on lens comfort and wettability by adding a thin coating to a standard silicone hydrogel. While the reported oxygen permeability and modulus values appear slightly different with the coating application, this is not statistically significant and is within the noise of repeated measurements. Moreover, these differences were low compared to the range of these parameters across currently available commercial soft contact lenses.

Lens comfort was significantly greater with the coated than the uncoated soft contact lenses, reaching levels previously reported in a general population without lens wear (34). The self-reported comfort did not significantly vary with time of day, although lens comfort was slightly better in the middle of the day than immediately on insertion or at the end of the day as expected (4-8). The symptoms of dryness also reduced with lens coating from levels considered to be dry eye to sub-threshold (35, 36). Tear breakup time on the surface of a contact lens has been shown to be around five to six seconds over a soft contact lens (37) due to a thinner lipid layer thickness (38, 39). In this study, the values were similar for pre-lens tear film stability of the uncoated lenses. It is important to consider that tear film stability of the ocular surface is generally shorter when measured by objective compared to subjective techniques (40). Since our tear breakup time values for one months' wear of coated lenses were close to subjective studies in a similarly aged cohort (41), lens wettability with coating lens wear seems not only better than in the studied uncoated silicone hydrogels, but also may be considerably greater compared to other commercial available contact lenses. This level of coated lens performance is reached within one week and maintained over a full month of daily wear. However, as has been shown previously, in-vivo wettability is not directly associated with differences in subjectively rated comfort between lenses or individuals (6). Moreover, the fact that NIKBUT averages values were greater in coated than uncoated lenses suggests that the application of a lens coating may change the

behaviour of the pre-lens tear film, postponing the lens surface dewetting to values even higher than those measured in a healthy population who have not worn contact lenses in the past 24 hours (42). With respect to subjects' ocular health, bulbar and limbal redness was low as is expected with silicone hydrogel soft contact lens wear and was unaffected by the lens coating (43). In our study though, the use of hydrogen peroxide as cleaning system, which has shown to cause less levels of hyperaemia than other preserved multipurpose solutions (44), may have masked any possible bulbar and limbal redness due to the friction between the lens surface and lid margin.

In conclusion, changing the physical properties (lubricity) of just the surface of a soft contact lens does impact subjectively rated comfort as previously hypothesised (26), which in turn should result in reduced contact lens discontinuation. Further studies are needed to determine how linear is the relationship between lens surface lubricity and ocular comfort, as well as the possible impact of lens handling.

Acknowledgments

This work received funding by EU Horizon 2020 research and innovation programme under Marie Skłodowska-Curie grant agreement [grant number 642760]. Lenses and coating was provided by Bettervision Pty, Keller, TX, USA.

Conflicts of interest

We have no conflict of interest to declare.

References

1. K. Dumbleton, B. Caffery, M. Dogru, S. Hickson-Curran, J. Kern, T. Kojima, P.B. Morgan, C. Purslow, D.M. Robertson, J.D. Nelson; members of the TFOS International Workshop on Contact Lens Discomfort. I. The TFOS International Workshop on Contact Lens Discomfort: report of the subcommittee on epidemiology. *Invest Ophthalmol Vis Sci.* 54 (2013) 20-36.
2. J.J. Nichols, M.D. Willcox, A.J. Bron, C. Belmonte, J.B. Ciolino, J.P. Craig, M. Dogru, G.N. Foulks, L. Jones, J.D. Nelson, K.K. Nichols, C. Purslow, D.A. Schaumberg, F. Stapleton, D.A. Sullivan; members of the TFOS International Workshop on Contact Lens Discomfort.. The TFOS International Workshop on Contact Lens Discomfort: executive summary. *Invest Ophthalmol Vis Sci.* 54 (2013) 7-13.
3. K.A. Dumbleton, M. Guillon, P. Theodoratos, T. Patel. Diurnal variation in comfort in contact lens and non-contact lens wearers. *Optom Vis Sci.* 93 (2016) 820-827.
4. C.G. Begley, B. Caffery, K.K. Nichols, R. Chalmers. Responses of contact lens wearers to a dry eye survey. *Optom Vis Sci.* 77 (2000) 40-46.
5. R.L. Chalmers, C.G. Begley. Dryness symptoms among an unselected clinical population with and without contact lens wear. *Cont Lens Anterior Eye.* 29 (2006) 25-30.
6. J.S. Wolffsohn, S. Mroczkowska, O.A. Hunt, P. Bilkhu, T. Drew, A. Sheppard. Crossover evaluation of silicone hydrogel daily disposable contact lenses. *Optom Vis Sci.* 92 (2015) 1063-1068.
7. C.G. Begley, R.L. Chalmers, G.L. Mitchell, K.K. Nichols, B. Caffery, T. Simpson, R. DuToit, J. Portello, L. Davis. Characterization of ocular surface symptoms from optometric practices in North America. *Cornea* 20 (2001) 610-618.
8. J.J. Nichols, G.L. Mitchell, K.K. Nichols, R. Chalmers, C. Begley. The performance of the contact lens dry eye questionnaire as a screening survey for contact lens-related dry eye. *Cornea* 21 (2002) 469-475.
9. M. Guillon, C. Maissa. Dry eye symptomatology of soft contact lens wearers and nonwearers. *Optom Vis Sci.* 82 (2005) 829-834.
10. J.J. Nichols, C. Ziegler, G.L. Mitchell, K.K. Nichols. Self-reported dry eye disease across refractive modalities. *Invest Ophthalmol Vis Sci.* 46 (2005) 1911-1914.
11. E.B. Papas, D. Tilia, D. Tomlinson, J. Williams, E. Chan, J. Chan, B. Golebiowski. Consequences of wear interruption for discomfort with contact lenses. *Optom Vis Sci.* 91 (2014) 24-31.
12. M.J. Glasson, F. Stapleton, L. Keay, D. Sweeney, M.D. Willcox. Differences in clinical parameters and tear film of tolerant and intolerant contact lens wearers. *Invest Ophthalmol Vis Sci.* 44 (2003) 5116-5124.
13. E. Faber, T.R. Golding, R. Lowe, N.A. Brennan. Effect of hydrogel lens wear on tear film stability. *Optom Vis Sci.* 68 (1991) 380-384.

14. M. Glasson, S. Hseuh, M. Willcox. Preliminary tear film measurements of tolerant and non-tolerant contact lens wearers. *Clin Exp Optom*. 82 (1999) 177-181.
15. J.J. Nichols, L.T. Sinnott. Tear film, contact lens, and patient-related factors associated with contact lens-related dry eye. *Invest Ophthalmol Vis Sci*. 47 (2006) 1319-1328.
16. R. Arita, K. Itoh, K. Inoue, A. Kuchiba, T. Yamaguchi, S. Amano. Contact lens wear is associated with decrease of meibomian glands. *Ophthalmology*. 116 (2009) 379-384.
17. C.W. McMonnies, A. Chapman-Davies. Assessment of conjunctival hyperemia in contact lens wearers. Part I. *Optom Vis Sci*. 64 (1987) 246-250.
18. M. Guillon, C. Maissa. Bulbar conjunctival staining in contact lens wearers and non lens wearers and its association with symptomatology. *Cont Lens Anterior Eye*. 28 (2005) 67-73.
19. J.J. Nichols, L.T. Sinnott. Tear film, contact lens, and patient factors associated with corneal staining. *Invest Ophthalmol Vis Sci*. 52 (2011) 1127-1137.
20. K.K. Nichols, G.L. Mitchell, K.M.S. Simon, D.A. Chivers, T.B. Edrington. Corneal staining in hydrogel lens wearers. *Optom Vis Sci*. 79 (2002) 20-30.
21. K.K. Nichols, J.J. Nichols, G.L. Mitchell. The lack of association between signs and symptoms in patients with dry eye disease. *Cornea*. 23 (2004) 762-770.
22. D.K. Martin. Water transport in dehydrating hydrogel contact lenses: implications for corneal desiccation. *J Biomed Mater Res A*. 29 (1995) 857-865.
23. P. McConville, J.M. Pope. Diffusion limited evaporation rates in hydrogel contact lenses. *Eye & Contact Lens*. 27 (2001) 186-191.
24. N. Efron, N.A. Brennan, J.M. Currie, J.P. Fitzgerald, M.T. Hughes. Determinants of the initial comfort of hydrogel contact lenses. *Optom Vis Sci*. 63 (1986) 819-823.
25. G. Young. Evaluation of soft contact lens fitting characteristics. *Optom Vis Sci*. 73 (1996) 247-254.
26. L. Jones, N.A. Brennan, J. González-Méijome, J. Lally, C. Maldonado-Codina, T.A. Schmidt, L. Subbaraman, G. Young, J.J. Nichols; members of the TFOS International Workshop on Contact Lens Discomfort. al. The TFOS International Workshop on Contact Lens Discomfort: report of the contact lens materials, design, and care subcommittee. *Invest Ophthalmol Vis Sci*. 54 (2013) 37-70.
27. G. Ross, M. Nasso, V. Franklin, F. Lydon, B. Tighe. Silicone hydrogels: trends in products and properties. Poster presented at: BCLA 29th Clinical Conference & Exhibition; June 3-5, 2005; Brighton, UK. Available at: http://www.siliconehydrogels.org/pdf/posters/dec_05/Tighe_BCLA2005.pdf. Accessed Sep 9, 2017.
28. N. Brennan. Contact lens-based correlates of soft lens wearing comfort. *Optom Vis Sci*. 86 (2009) e-abstract 90957.

29. M. Roba, E.G. Duncan, G.A. Hill, N.D. Spencer, S.G.P. Tosatti. Friction measurements on contact lenses in their operating environment. *Tribol Lett.* 44 (2011) 378-397.
30. J.S. Wolffsohn, O.A. Hunt, A.K. Basra. Simplified recording of soft contact lens fit. *Cont Lens Anterior Eye.* 32 (2009) 37-42.
31. S. Wu, J. Hong, L. Tian, X. Cui, X. Sun, J. Xu. Assessment of bulbar redness with a newly developed keratograph. *Optom Vis Sci.* 92 (2005) 892-899.
32. R.A. Armstrong, F. Eperjesi, B. Gilmartin. The application of analysis of variance (ANOVA) to different experimental designs in optometry. *Ophthal Physiol Opt.* 22 (2002) 248-256.
33. C. Coles, N. Brennan. Coefficient of friction and soft contact lens comfort. *Optom Vis Sci.* 88 (2012) e-abstract 125603.
34. W. Li, A.D. Graham, M.C. Lin. Understanding ocular discomfort and dryness using the pain sensitivity questionnaire. *Plos One.* 11 (2016) e0154753.
35. G. Young, R.L. Chalmers, L. Napier, C. Hunt, J. Kern. Characterizing contact lens-related dryness symptoms in a cross-section of UK soft lens wearers. *Cont Lens Anterior Eye.* 34 (2011) 64-70.
36. R.L. Chalmers, G. Young, J. Kern, L. Napier, C. Hunt. Soft Contact lens-related symptoms in North America and the United Kingdom. *Optom Vis Sci.* 93 (2016) 836-847.
37. C.A. Morris, B.A. Holden, E. Papas, H.J. GriesserJ, S. Bolis, P. Anderton, F. Carney. The ocular surface, the tear film, and the wettability of contact lenses. *Adv Exp Med Biol.* 438 (1998) 717-722.
38. M. Guillon, J.P. Guillon. Hydrogel lens wettability during overnight wear. *Ophthal Physiol Opt.* 9 (1989) 355-359.
39. G. Young, N. Efron. Characteristics of the pre-lens tear film during hydrogel contact lens wear. *Ophthal Physiol Opt.* 11 (1991) 53-58.
40. N. Best, L. Drury, J.S. Wolffsohn. Clinical evaluation of the Oculus Keratograph. *Cont Lens Anterior Eye.* 35 (2012) 171-174.
41. W. Lan, L. Lin, X. Yang, M. Yu. Automatic noninvasive tear breakup time (TBUT) and conventional fluorescent TBUT. *Optom Vis Sci.* 91 (2014) 1412-1418.
42. L. Tian, J.H. Qu, X.Y. Zhang, X.G. Sun. Repeatability and reproducibility of noninvasive Keratograph 5M measurements in patients with dry eye disease. *J Ophthalmol.* 2016 (2016) 8013621.
43. A. Sivardeen, D. Laughton, J.S. Wolffsohn. Randomized crossover trial of silicone hydrogel presbyopic contact lenses. *Optom Vis Sci.* 93 (2016) 141-149.
44. G. Young, N. Keir, C. Hunt, C.A. Woods. Clinical evaluation of long-term users of two contact lens care preservative systems. *Eye and Contact Lens.* 35 (2009) 50-58.